

Audio-HA® Adjustable Partial Prosthesis

CODE
TPL 07.08

HA: Bioactive calcium hydroxylapatite ceramic

It replaces the incus or the incudo-malleolar block.


The interposition of cartilage or bone paste between the flange and the tympanic membrane is not required.

The columella is joined to the flange by means of a platinum segment.

Platinum is known to be malleable and bioinert (tolerable).

The malleable segment allows duplication of the angle between the tympanic membrane and the columella and movement of the columella further off-center so that it is perpendicular to the head of the stapes, thus centering the stapes in the oval window.

The flange can be bound to the tympanic membrane by fibrine glue.

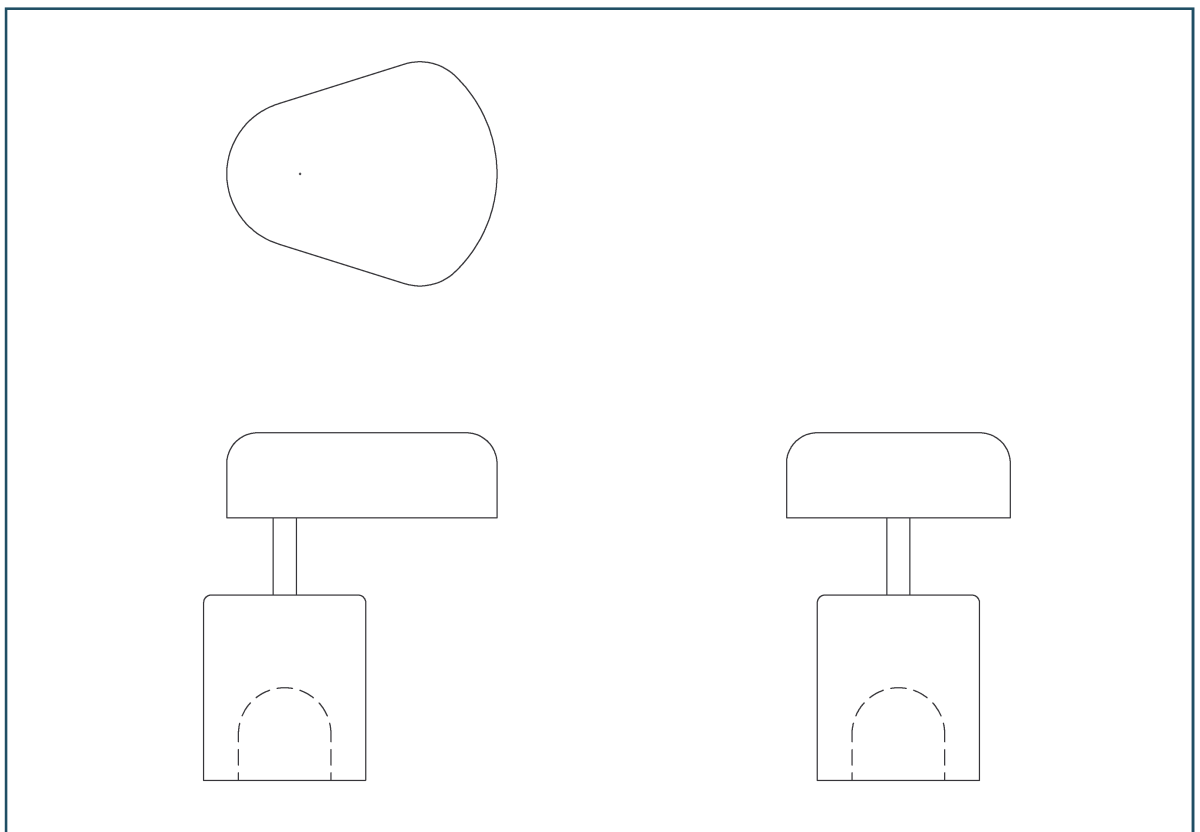


Dimensions

Total length (mm):
3.50 - 4.00 - 4.50
5.00 - 5.50 - 6.00
Flange maximum length: 3.60 mm
Flange thickness: 1.00 mm
Columella outside diameter: 2.00 mm
Columella inside diameter: 1.20 mm

Packaging

Dispenser box containing 6 sterile,
individually packaged implants.

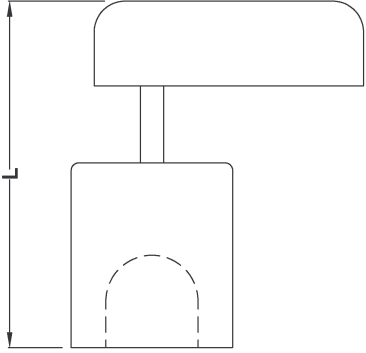	Total length (L) mm	Code
	3.50	TPL 07.08.350
	4.00	TPL 07.08.400
	4.50	TPL 07.08.450
	5.00	TPL 07.08.500
	5.50	TPL 07.08.550
	6.00	TPL 07.08.600

